




Analysis of ascorbic acid, citric acid and benzoic acid in orange juice

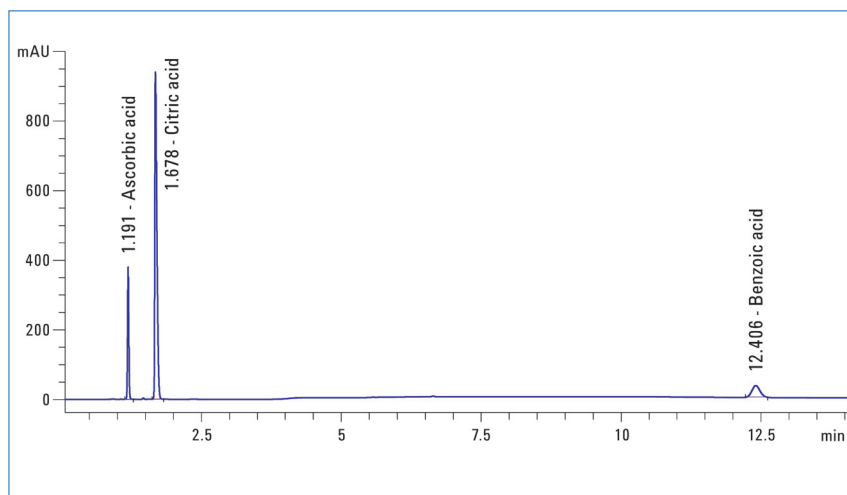

Application Solution

- Method development
- Method validation
- Sample preparation
- Real-life sample analysis

Abstract

Food additives, such as antioxidants and preservatives, are added to increase the shelf life of food items. In this Application Solution, we describe a method to quantify an antioxidant (vitamin C) and preservatives (citric acid, benzoic acid) in orange juice. The method was developed on the Agilent 1260 Infinity LC system using an Agilent Poroshell EC-C18 column. During sample recovery studies, greater than 90% recovery was obtained for all the three compounds. The method was effectively converted to a short UHPLC method using an Agilent 1290 Infinity LC system. This new method was 5x faster with the same LOD for benzoic acid. Both methods can be effectively applied by food manufacturers for quality control of food additives.



Scope and Benefits

Antioxidants, such as ascorbic acid prevent oxidation by decreasing the available oxygen in the environment. Preservatives, such as citric acid or benzoic acid prevent or inhibit the growth of microorganisms in food. Although the regulatory limit for benzoic acid in fruit juices is 400 to 600 µg/mL there are concerns about the liberation of carcinogenic benzene by reaction of benzoic acid with ascorbic acid under certain conditions.

The AOAC Official Method 994.11 shows the UV-based detection of benzoic acid in orange juice. In this Application Solution we describe a method to simultaneously quantify ascorbic acid, citric acid and benzoic acid using UV based detection and a simple extraction procedure.

Analytes

Ascorbic acid, Benzoic acid, Citric acid

Matrix

Orange juice

Ordering Information



Agilent 1260 Infinity Binary LC

Description

- 1260 Infinity Binary Pump
- 1260 Infinity Vacuum Degasser
- 1260 Infinity High performance Autosampler with Thermostat
- 1260 Infinity Thermostatted Column Compartment
- 1260 Infinity Diode Array Detector

Part Number

G1312B
G1379B
G1367E
G1330B
G1316A
G4212B

Agilent 1290 Infinity LC

Description

- 1290 Infinity Binary Pump with integrated vacuum degasser
- 1290 Infinity High Performance Autosampler with Thermostat
- 1290 Infinity Thermostatted Column Compartment
- 1290 Infinity Diode Array Detector

Part Number

G4220A
G4226A
G1330B
G1316C
G4212A

Software

Agilent ChemStation B.04.03 or higher

Columns

Description

ZORBAX Poroshell 120 EC-C18 4.6 x 100 mm, 2.7 µm

Part Number

697975-302

Chemicals

HPLC grade solvents

All chemicals were purchased from regular suppliers

For full details of this application see

Agilent Application Note 5990-8720EN

www.agilent.com/chem/lc

© Agilent Technologies, Inc. 2011
Published in Germany September 1, 2011
5990-9033EN



Agilent Technologies