

Analysis of Plasma Proteome for a Respiratory Disease Cohort Using SONAR on a SYNAPT XS Mass Spectrometer

Christopher Hughes,¹ Lee Gethings,¹ Joanne Ballantyne,¹ and Robert Plumb²

¹Micromass UK Limited, Wilmslow, Cheshire, UK; ²Waters Corporation, Milford, MA, USA



The demonstration of SONAR on a SYNAPT XS platform to analyze the plasma proteome.

GOAL

The application of SONAR™ on a SYNAPT™ XS platform for improved specificity, higher sequence coverage, and increased confidence in identification following database search.

BACKGROUND

Traditionally, proteomics has used data dependent (DDA) strategies for mass spectrometry (MS) acquisition. However, developments in data independent (DIA) modes of acquisition have provided the ability to gain qualitative and quantitative information in a single injection without the drawbacks associated with DDA workflows. Several DIA variants exist, but an alternative approach is to apply a DIA methodology that allows for high throughput whilst ensuring high specificity and quantitative accuracy. SONAR has previously been described,^{1,2} highlighting the utilization of a fast scanning quadrupole, enabling the technique to be compatible with fast chromatography and high-throughput workflows. Here, we present the applicability

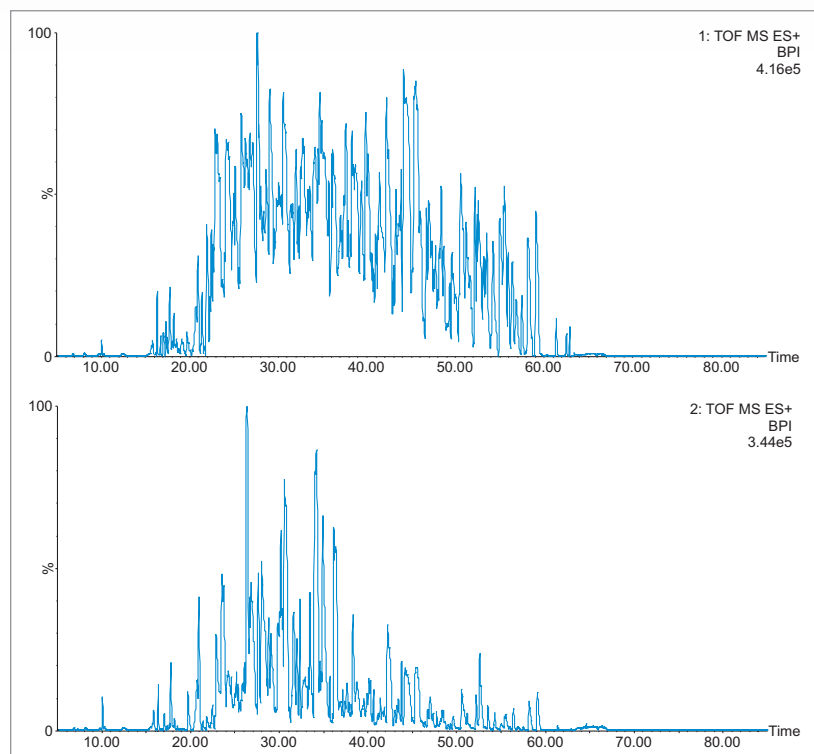


Figure 1. Representative chromatograms corresponding to the control cohort plasma for precursor/low energy data (upper chromatogram) and fragment/high energy data (lower chromatogram).

of SONAR on a SYNAPT XS platform for the identification and relative quantification of plasma proteins from a patient cohort consisting of controls, chronic obstructive pulmonary disease (COPD), and asthma.

THE SOLUTION

The analyzed samples consisted of tryptically digested, undepleted human plasma from three different conditions. Sample groups consisted of controls (n=6), chronic obstructive pulmonary disease (n=6), and asthma (n=6). Individual samples per group were pooled to provide three working samples.

Peptides were separated using an ACQUITY™ UPLC™ M-Class System, which was equipped with an ACQUITY UPLC Peptide CSH C₁₈, 300 μm I.D. × 100 mm long analytical column. Samples were analyzed in triplicate (QC=5 injections) based on 5 μg loadings. The samples were separated using a reversed-phase gradient from 1 to 40% acetonitrile (+0.1% formic acid) over 45 minutes at a flow rate of 50 μL/min. Data were collected using a SYNAPT XS which operated using the SONAR mode of acquisition. Data were processed using Progenesis™ QI for Proteomics and database searched against a human database, consisting of UniProt reviewed sequences. Searches were performed using carbamidomethyl C (fixed) and oxidation of methionine (variable) modifications in addition to a 1% FDR.

Example chromatograms representing SONAR acquisition are shown in Figure 1 for both precursor and fragment ion data. The benefits of high selectivity when implementing SONAR have previously been reported.^{1,2} Figure 2 shows the enhanced specificity provided by the scanning quadrupole implemented for increased peptide identification. Data processing with Progenesis QI for Proteomics identified a total of 349 proteins with the majority of identifications overlapping between all three cohorts (Figure 3A), whilst the median sequence coverage achieved varied between 18–25% across groups (Figure 3B). The ability to reproducibly identify and quantify analytes of interest is important to ensure consistency over the analysis. Figure 3C shows the coefficient of variation (CV) for the normalized abundance across technical replicates for each condition, with a median CV less than 3% being achieved across each condition. Furthermore, a linear dynamic range of 3–4 orders magnitude is demonstrated for each condition (Figure 4).

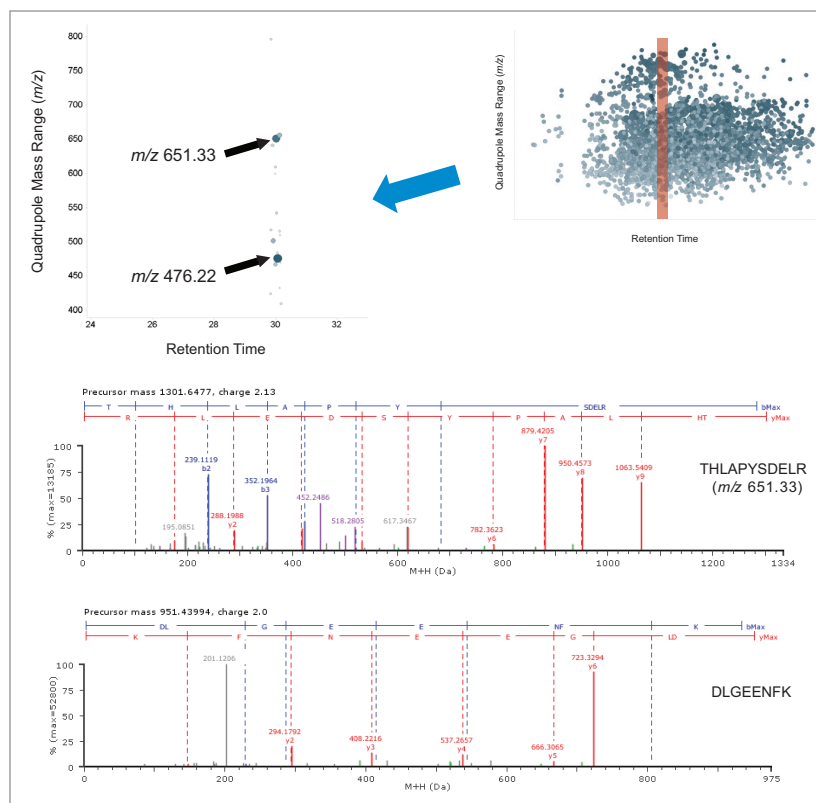


Figure 2. Increased specificity provided by SONAR. Co-eluting peptides related to ApoA1 (THLAPYSDELRL, m/z 651.33) and Albumin (DLGEENFK, m/z 476.22) show clear separation based on the scanning quadrupole dimension. Resulting MS2 spectra for both example peptides are shown, providing enhanced clarity and increased identification confidence.

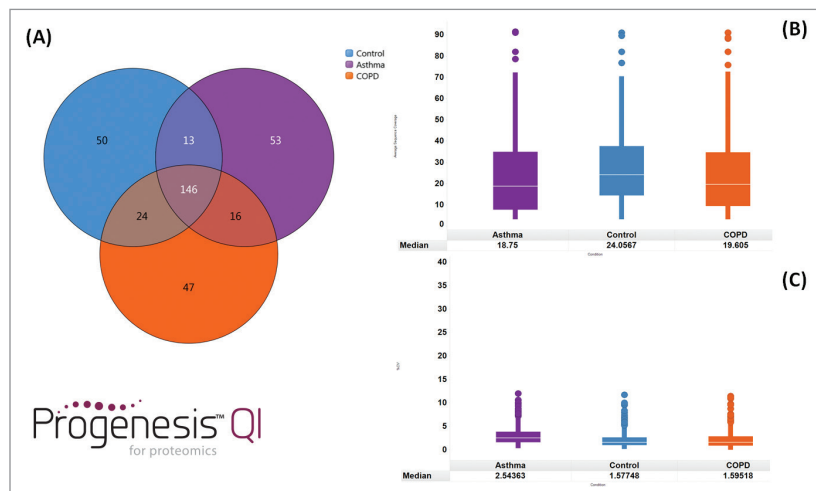


Figure 3. Protein overview for the three cohorts. Venn diagram indicates that most of the proteins overlap between conditions (A), while box-whisker plots show the technical reproducibility of the SONAR technique in terms of protein sequence coverage (B) and % CV (C).

The ability to integrate data with third-party informatics is integral for flexibility and comprehensive data analysis. SONAR generated data is compatible with a variety of software tools and is demonstrated within this study using Skyline software (Figure 5), highlighting serotransferrin as an example protein with associated peptide transitions.

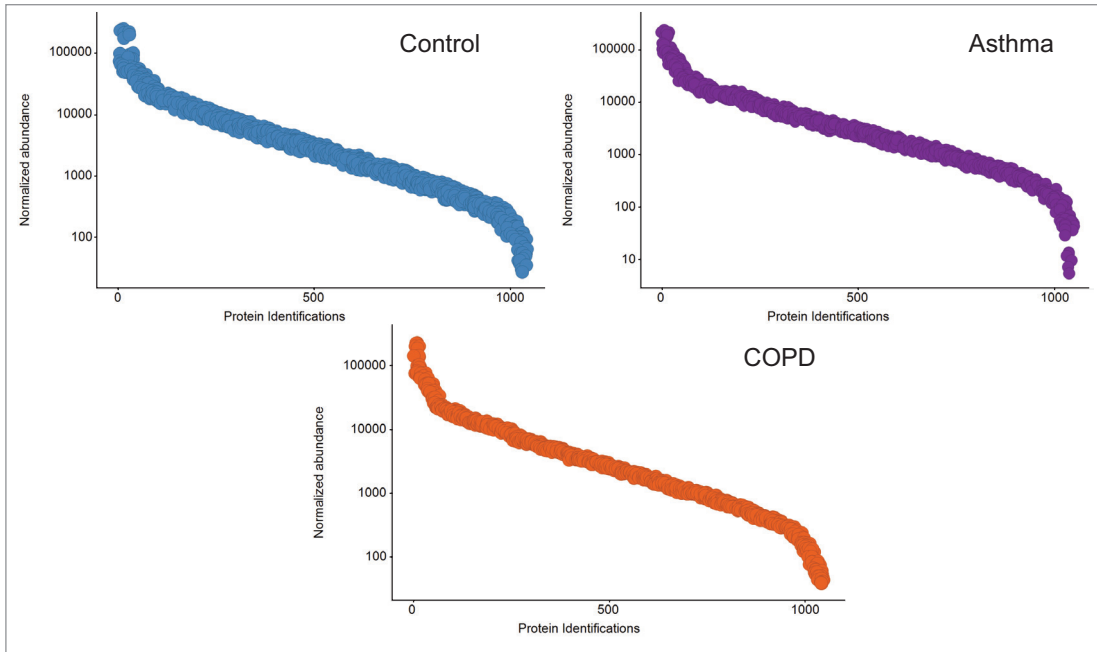


Figure 4. Observed dynamic range measured for each biological condition. Control (blue), asthma (purple), and COPD (orange) cohorts exhibit over 3–4 orders linear dynamic range. Each of the conditions shown comprise of all three technical replicates.

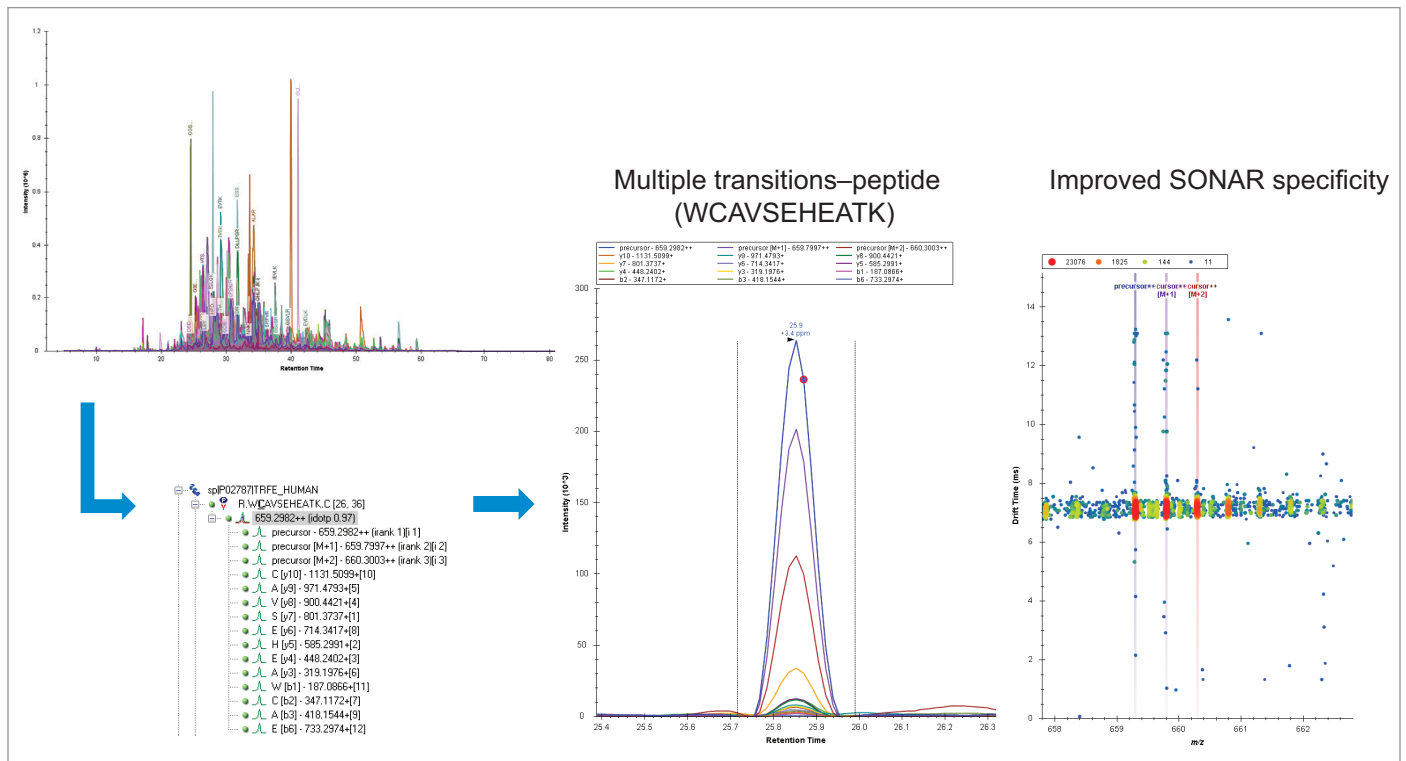


Figure 5. Integration of SONAR data with Skyline. A representative peptide (WCAVSEHEATK) corresponding to serotransferrin shows high quantitative accuracy with over 10 points across the chromatographic peak. Multiple peptide transitions are clearly identified along with the benefits of increased specificity from SONAR.

SUMMARY

We have shown the utility of SONAR on a SYNAPT XS platform for the proteomic analysis of plasma originating from a respiratory disease patient cohort. Implementing a SONAR acquisition workflow has shown high specificity, wide dynamic range, high protein identification, and sequence coverage. Processing the data through Progenesis Q1 for Proteomics and other third-party tools, highlights the flexibility of the SONAR workflow. These benefits have been demonstrated with a proteomics example, however the benefits can also be applied to metabolomics and lipidomics for multi-omic-based studies.

References

1. Gethings, L.A.; et al. Lipid profiling of complex biological mixtures by liquid chromatography/mass spectrometry using a novel scanning quadrupole data-independent acquisition strategy. *Rapid Commun Mass Spectrom.* **2017**, *31*(19), 1599–1606. doi: 10.1002/rcm.7941.
2. Moseley, A.M.; et al. Scanning quadrupole data independent acquisition – part A. Qualitative and quantitative characterization. *J. Proteome Res.* **2017**, *17*(2), 770–779. doi: 10.1021/acs.jproteome.7b00464.

Waters

THE SCIENCE OF WHAT'S POSSIBLE.™

Waters, The Science of What's Possible, SONAR, SYNAPT, ACQUITY, UPLC, and Progenesis are trademarks of Waters Corporation. All other trademarks are the property of their respective owners.

©2019 Waters Corporation. Produced in the U.S.A. August 2019 720006598EN AG-PDF

Waters Corporation
34 Maple Street
Milford, MA 01757 U.S.A.
T: 1 508 478 2000
F: 1 508 872 1990
www.waters.com