

MetaboQuan-R for the Analysis of Tryptophan and its Metabolites

Billy Joe Molloy
Waters Corporation, Wilmslow, UK

APPLICATION BENEFITS

- Simultaneous analysis of tryptophan and seven of its metabolites in a single analytical run in less than three minutes
- High-throughput analysis means larger sample sets can be analyzed quickly
- Use of a generic LC-MS configuration provides the versatility of switching from one compound class to another

WATERS SOLUTIONS

[CORTECS™ UPLC™ Column](#)

[OASIS™ PRiME HLB \$\mu\$ Elution Plate](#)

[ACQUITY™ UPLC I-Class System](#)

[Xevo™ TQ-S micro Mass Spectrometer](#)

[MassLynx™ Software](#)

[TargetLynx Software](#)

[Quanpedia™ Database](#)

KEYWORDS

Targeted omics, tryptophan, UPLC, CORTECS, tandem quadrupole, Xevo TQ-S micro, multiple reaction monitoring (MRM), metabolomics

INTRODUCTION

Tryptophan is an amino acid that, along with its metabolites (Figure 1), plays a crucial role in a variety of biological functions, including brain health and cardiometabolic regulation. As such, the study of tryptophan metabolism is of interest in biomedical research, and a high-throughput analytical method for the analysis of tryptophan and its metabolites enables the analysis of large cohort studies. Presented here is a high-throughput UPLC method that utilizes a flexible LC-MS platform. The method can be used seamlessly alongside methods for other compound classes contained in the [Targeted Omics Method Library](#) and enables labs to easily and conveniently increase analyte coverage without the burden of method development.

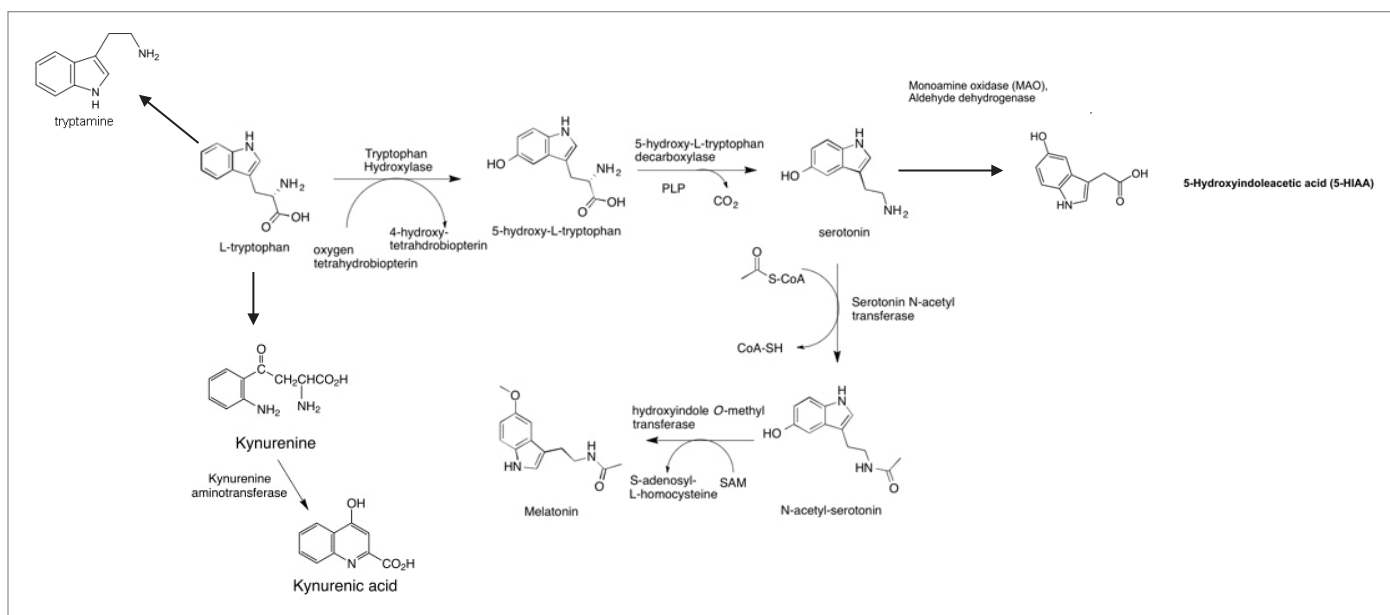


Figure 1. Schematic showing the metabolic pathway for tryptophan.

EXPERIMENTAL

Sample preparation

Human urine

One hundred microliters of human urine were diluted 1:10 with 900 μL of LC-MS-grade water. One microliter of this was then injected onto the UPLC-MS/MS system.

Human plasma

One hundred fifty microliters of human plasma were extracted using solid-phase extraction (SPE). Prior to extraction, the samples were centrifuged so that they would not block the SPE plate. A 150- μL aliquot of each sample was then diluted with 450 μL of water before loading onto an Oasis HLB PRiME $\mu\text{Elution}$ Plate. The plate was then washed with 150 μL of water. The analytes were eluted from the SPE plate using 25 μL of methanol. The eluate was then diluted 1:1 with 25 μL of water before injecting 1 μL onto the UPLC-MS/MS system.

LC conditions

UPLC separation was performed with an ACQUITY UPLC I-Class System (Fixed Loop), equipped with a CORTECS T3, 2.7 μm (2.1 \times 30 mm) Analytical Column. One microliter of sample was loaded onto the column and eluted under gradient conditions at a flow rate of 0.45 mL/min. Mobile phase A was 0.01% formic acid_(aq) and mobile phase B was 50% isopropanol

in acetonitrile containing 0.01% formic acid. After an initial 0.75-minute hold at 0% mobile phase B, tryptophan and its associated metabolites were eluted from the column and separated with a gradient of 0–70% mobile phase B over 0.95 minutes, followed by a one-minute column wash at 98% mobile phase B. The column was then re-equilibrated to initial conditions. The analytical column temperature was maintained at 60 $^{\circ}\text{C}$.

MS conditions

The analytes were detected using multiple reaction monitoring (MRM) analyses using a Xevo TQ-S micro Mass Spectrometer. All experiments were performed in positive electrospray ionization (ESI+) mode. The ion source temperature and capillary voltage were kept constant and set to 150 $^{\circ}\text{C}$ and 2.0 kV, respectively. The cone gas flow rate was 50 L/hr and desolvation temperature was 650 $^{\circ}\text{C}$.

Informatics

Method information was imported onto the LC-MS system using the Quanpedia functionality within MassLynx. This extendable and searchable database produces LC and MS methods, as well as processing methods, for use in TargetLynx for compound quantification.

RESULTS AND DISCUSSION

Tryptophan and its metabolites were separated and detected using the LC-MS platform and extraction protocols described above. Figure 2 shows an example chromatogram for the separation achieved using the method in a human urine sample. Peak identifications were confirmed using analytical standards. All analytes detailed in Table 1 were detected in human urine except for melatonin. Three analytes (serotonin, tryptophan, and kynurenine) were detected in human plasma. In Table 1, only one MRM transition is listed for some analytes whereas multiple MRM transitions are listed for other analytes. Both single and multiple MRMs gave similar levels of sensitivity. All the transitions were included for increased specificity.

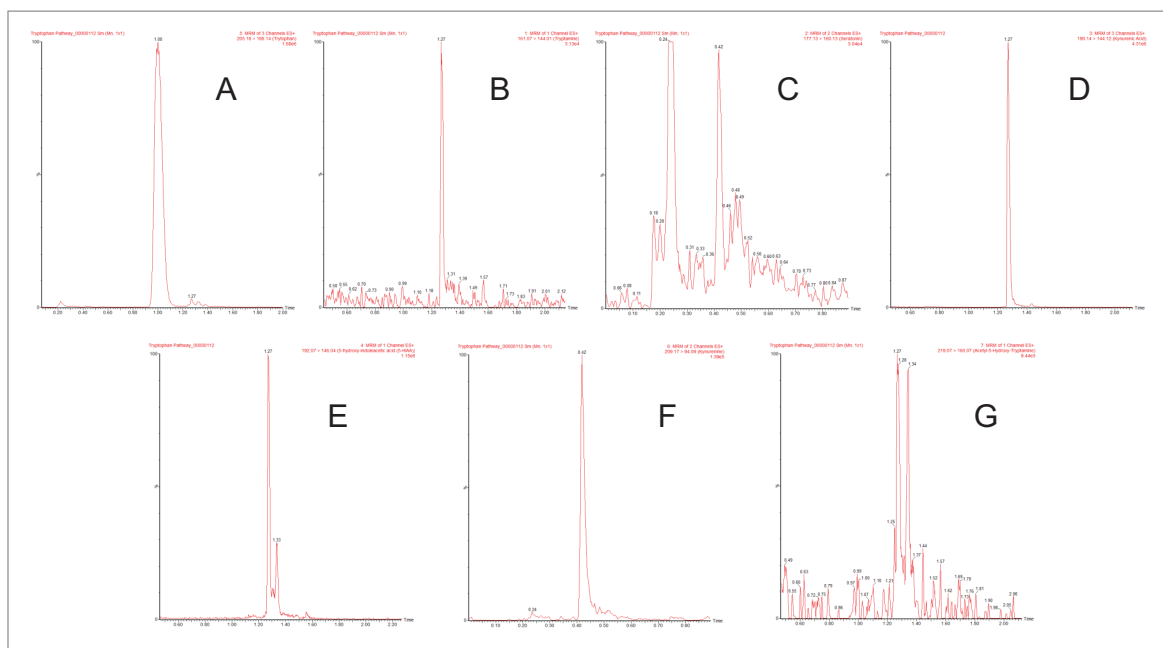


Figure 2. Typical chromatograms for tryptophan and its metabolites in human urine using the MetaboQuan-R™ platform: (A) tryptophan, (B) tryptamine, (C) serotonin, (D) kynurenic acid, (E) 5-HIAA, (F) kynurenine, (G) acetyl-5-hydroxy-tryptamine.

Table 1. MS-MS conditions and retention times for tryptophan and its metabolites.

Analyte	MRM transitions	RT (min)	Cone voltage (V)	Collision energy (eV)
Tryptophan	205.17 > 118.11	1.00	20	24
	205.17 > 118.11		20	16
	205.17 > 118.11		20	10
Kynurenic acid	190.14 > 89.08	1.27	40	34
	190.14 > 116.11		40	30
	190.14 > 144.12		40	15
Kynurenine	209.17 > 94.09	0.42	20	12
	209.17 > 192.14		20	6
Tryptamine	161.07 > 144.01	1.27	20	14
Serotonin	177.13 > 115.10	0.41	30	24
	177.13 > 160.13		30	9
Melatonin	233.15 > 174.12	1.41	4	13
5-Hydroxy-indole acetic acid (5-HIAA)	192.07 > 146.04	1.27	10	13
Acetyl-5-hydroxy-tryptamine	219.07 > 160.17	1.28	35	8

CONCLUSIONS

A rapid UPLC-MS/MS methodology has been developed for the analysis of tryptophan and seven of its metabolites in various matrices. This research method has been demonstrated to be suitable for the analysis of physiologically relevant levels of these analytes in human plasma and urine. This method utilizes a generic, flexible LC-MS platform that can be used for various compound classes (including metabolomics, lipidomics, and proteomics), meaning it can be applied as part of a suite of analyses that are run sequentially as part of a targeted multi-omics workflow.

Waters

THE SCIENCE OF WHAT'S POSSIBLE.™

Waters, The Science of What's Possible, ACQUITY, CORTECS, UPLC, Oasis, MassLynx, MetaboQuan-R, Quanpedia, and Xevo are trademarks of Waters Corporation. All other trademarks are the property of their respective owners.

©2019 Waters Corporation. Produced in the U.S.A. September 2019 720006667EN AG-PDF

Waters Corporation
34 Maple Street
Milford, MA 01757 U.S.A.
T: 1 508 478 2000
F: 1 508 872 1990
www.waters.com