

Analysis of Aromatics using Agilent J&W FactorFour VF-WAXms GC Columns

Application Note


Author

Helena Jacobse
Agilent Technologies, Inc.

Conditions

Technique: GC-FID
Column: VF-WAXms 60 m x 0.25 mm df =
0.25 μ m (part number CP9207)
Temperature: 55 °C to 150 °C with 4 °C/min
Carrier Gas: Helium, 2.0 bar

Injector: 250 °C, split 75 mL/min
Detector: 275 °C, FID
Sample Size: 0.1 μ L
Sample: 0.1 % (cyclohexane)

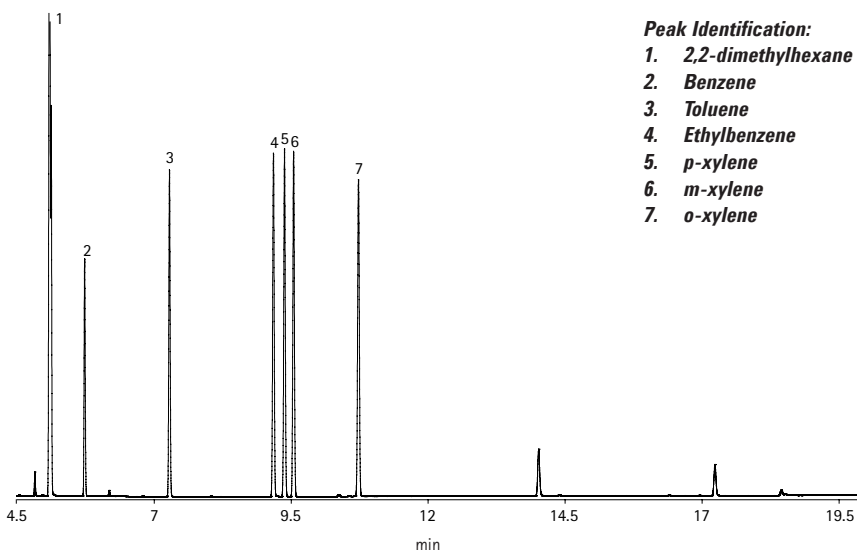

Analysis of aromatics using VF-WAXms GC columns

www.agilent.com/chem

This information is subject to change without notice.

© Agilent Technologies, Inc. 2010

Published in UK, October 08, 2010

SI-00938



Agilent Technologies