


Analysis of furnace oil in pentane

BP5

Column part number	054118		
Phase	BP5	Final temperature	350°C, 20 min
Column	12 m x 0.32 mm x 0.25 µm	Detector	FID
Initial temperature	100°C, 2 min	Injection mode	On-column
Rate	10°C/min	Carrier gas	H ₂ , 10 psi

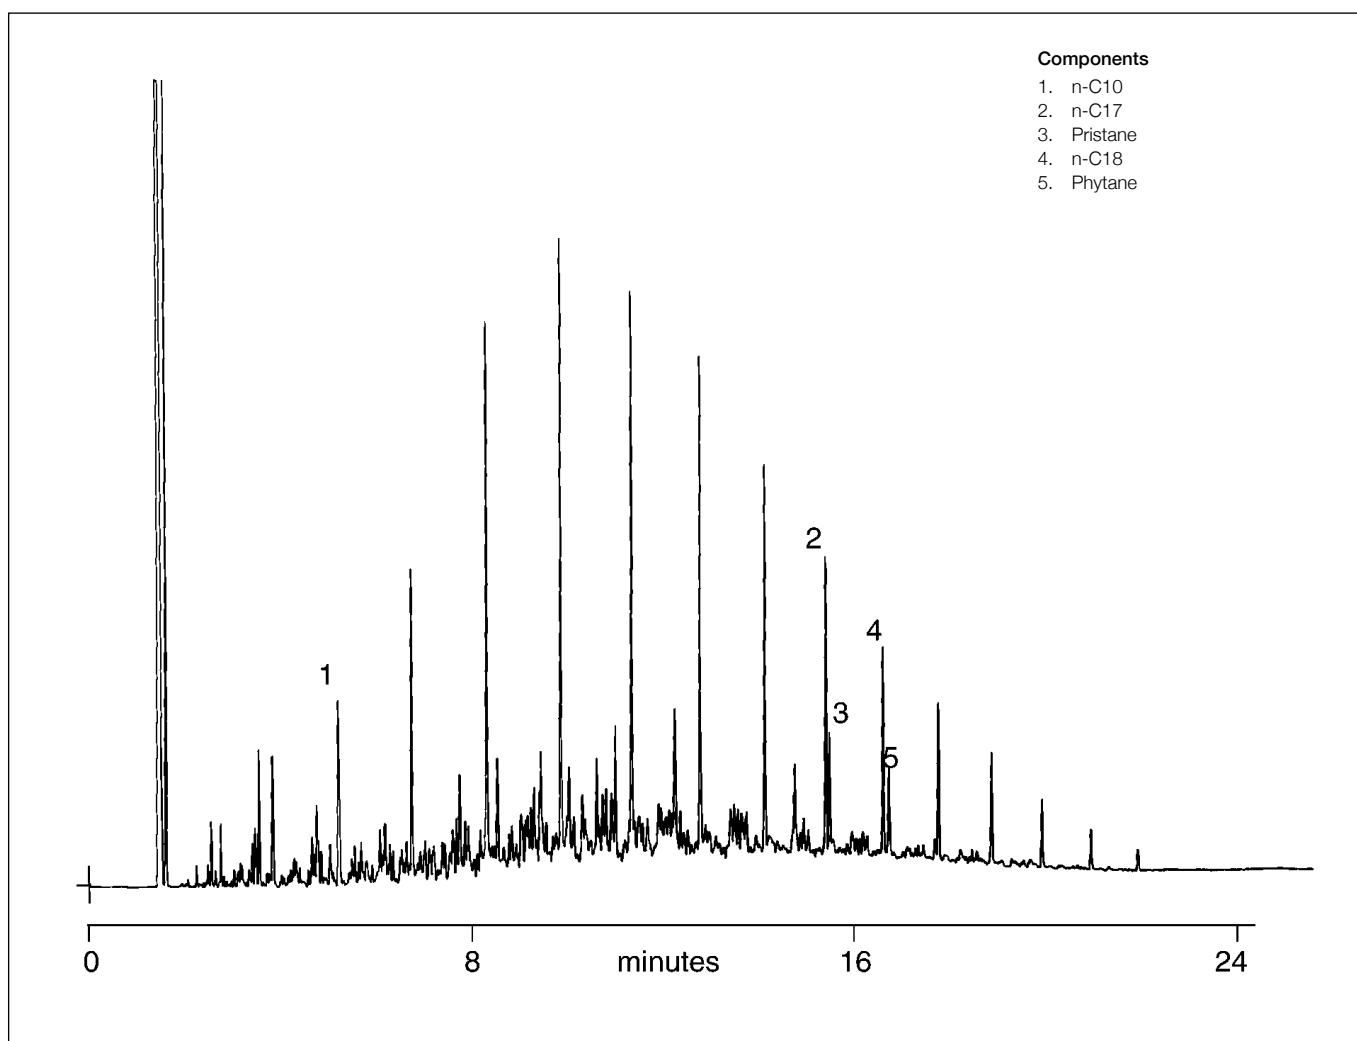

For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com