


## Analysis of food additives antimicrobials

**BP5**

Column part number	054186		
Phase	BP5	Detector	FID
Column	25 m x 0.32 mm x 0.5 µm	Sensitivity	256 x 10 <sup>-12</sup> AFS
Initial temperature	160°C, 0 min	Injection mode	Split
Rate	15°C/min	Carrier gas	H <sub>2</sub>
Final temperature	280°C, 0 min		

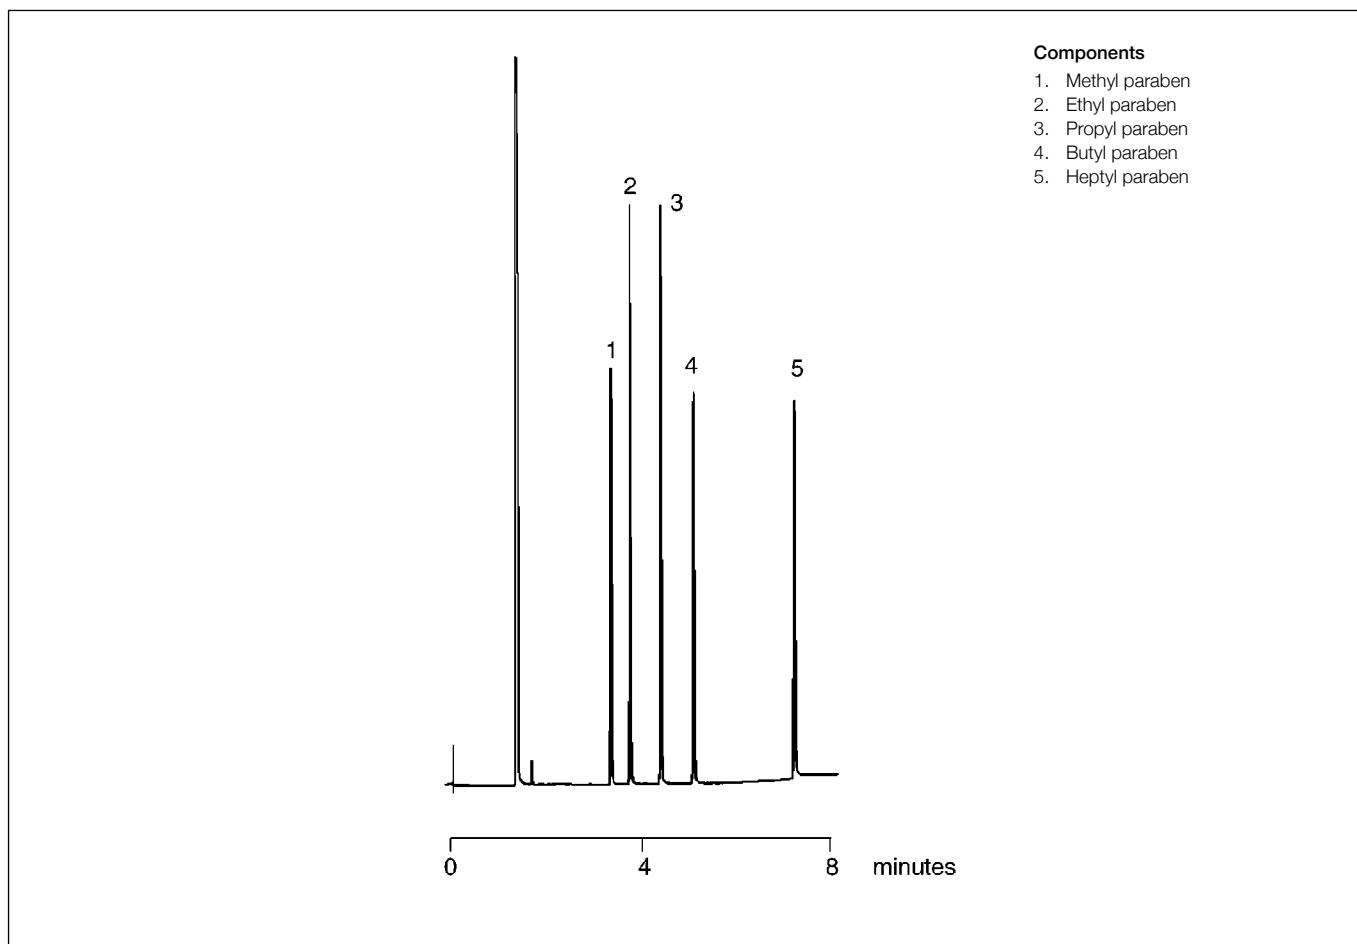

For more information visit [www.trajanscimed.com](http://www.trajanscimed.com) or contact [techsupport@trajanscimed.com](mailto:techsupport@trajanscimed.com)